

PFCO-Pharmacy-Machines

Standard Model: PFCO-PMA

Introduction

These unusual PFCO pharmacy machines are ideal for laboratory, hospital and clinic to compound a specific remedy for infectious lung disease. The specific remedy was to fixed dissolve some Ozone which pharmaceutical name shall be to denominate for PFCO-1, but it only suitable for clinical to put in use immediately or short-term store; another products for dissolve fixed some Oxygen to have other purpose of lung disease, the pharmaceutical name shall be to denominate for PFCO-2, it could be to store in a long-term.

These unusual PFCO pharmacy machines are consumption Fully-fluorinated liquid and the bottled Oxygen of purity over 99.5%.

The PFCO were specially for treating high fever from the SARS, bird flu and flu of any type including the phthisis, which advance at the same time has good effects on tidying up the lungs of smoker and lung-dust ill of aged people.

The invention of PFCO to put in used that was absolute to rewrite the history of medical treatment of Chinese and Western, so the PFCO medicine and the machine of pharmacy it will be about to obtain application extensively.

The machine of PFCO in accordance with the invent name that the "Surface Treatment of SARS-Infected Lungs" of the patent right of the HK patent number HK1060833 to supervise the manufacture and design, the patent right and copyright was possess simultaneously, so it must be strictly forbid to copy!

The patent application number of PCT was PCT/SG03/00145, the patent of every country in

PFCO-PMA



application; inventor is looking for the agent of the pharmacy machine or the PFCO medicine in every county.

Characteristics

- The standard model is PFCO-PMA which in used a set of ATI A15/64 dissolved ozone monitor, the measurement range it was enough for the pharmacy of PFCO-1 in general;
- The model of PFCO-PMB added one set of dissolved Oxygen monitor that measurement range between in 0-60ppm for pharmacy the PFCO-2 or to show the capacity of dissolved Oxygen of PFCO-1;
- The PFCO pharmacy machines was to pick an Ozone generator of water-cool type, the oxygen purity must to outstrip 99.5%;
- The PFCO pharmacy machines was made by stainless steel including the airtight-ness jar and it was inbuilt a filter in here;
- The standard airtight-ness jar to distinguish of three types which were 5, 10, 20 kilogram PFC which were 5, 10, 20 kilogram PFC capacity, to have something custom-made by order to specify;
- The PFCO pharmacy machines was to picked oil-less, non lubricated diaphragm liquid pump and control by a three digital timer for measure bottling or input the liquid for the lung transfusion bottle;
- The PFCO pharmacy machines was to pick the mix pump it could to prevent oxidation;
- The large-scale pharmacy machine include the automatic bottling system must by special quotation at some other time;
- Volume: 450 x 710 x 1360 mm (5Kgs)
- Pharmacy efficiency: 30-60 Min/ 5Kgs, it looks as if the standard of filter and consistency.
- Min. Pharmacy quantity: 1 kilogram
- Weight: 29 kilogram
- Overall Power: 146 watt / 220v

Equipment Introduction

1. A15/64 Dissolved Ozone Monitor:
 - a. Display: 16-character alphanumeric liquid crystal display with backlight.
 - b. Measurement Range: Programmable 0-20.00 PPM standard or 0-2.00.
 - c. Sensitivity: 0.001 PPM above 0.005 PPM
 - d. Repeatability: ± 0.01 PPM
 - e. Linearity: 0.5%
 - f. Response Time: 90% in <60 seconds
 - g. Output Range: Programmable for any range from 0-1 PPM to 0-20 PPM.
 - h. Sensor Temperature Compensation: Automatic -2°C to $+52^{\circ}\text{C}$.
 - i. Sensor: Polargraphic membraned sensor.
 - j. Sensor Materials: Noryl and stainless steel.
 2. Digital Timer: 0-999 second.
 3. Magnetic Drive Mix Pump:
 - a. Motor: 6 W / 220 VAC / 50 Hz
 - b. Speed: 2,800 rpm.
 4. Diaphragm Liquid Pump:
 - a. Free flow: 400 ml/min
 - b. Max. Power consumption: 5 W
 - c. Max. Suction height/vacuum: 6.0m WC
 - d. Max. Pressure intermit-tend: 15m WC
 - e. Max. Pressure continuous: 10 m WC
 5. Ozone generators:
 - a. Max. to yield up: 3g / h
 - b. Power: 80 watt / 220v AC
 6. One set of Cooling radiator:
 - a. Capacity: 400 x 90 x 250 mm
 - b. A submersible pump or pressure boost: 50 watt / 220vAC
 7. Customer have authority to choose to arrange for one set of destruct chamber for deal with the overflow for mix or discharge outdoor:
 - a. Power: 150 watt / 220v AC;
 - b. Catalyst Mixture: MnO₂/CuO;
 - c. Construction: T316 Stainless Steel;
 - d. The specifics after in order.
-


The PFCO is an up-to-date medicine of an invent patent, but, the Ozone can not be stored in the medicine to offer for sale, so the clinic and hospital who they must to buy the PFCO-1 machine and the patent to be authorized after that right away to compound and right away to use, the effect of medication far better than the present one by hundredfold which medicines of lung germs infect, for instance, As there is a need to define air as an interface, so SARS infection include any type of flu which is alike property of the ulcer of superficiality and bacterial infection, this is a new medical definition and as well as the basis of our patent invention and the basis for your belief in our patent too. It also that proven that the effect of medication of any antibiotics or vaccine was inevitable finite for bacterial infection of lung illness of any type flu, up to the present, no anyone doctor or specialist who could to negate this diagnosis theory of medical science! That was to include in before long time, a SARS medicine guides still to point those steroids, Ribavirin of antibiotics that make public of the Hong Kong Hospital Authority, obvious, the error in diagnosis was unlucky for residents of HK city! The requisition for patent negotiations it was still in proceed.

Therefore, the PFCO-1 was the only chosen medicine for curing SARS, this medicine machine can be used to control the Ozone concentration easily, the clinical concentration form it could be to consult "The effect of medication and ingredients of PFCO-1", the misgivings of "burn lung-cell" it may be solved by the hide-test, in addition to this, the clinical does not have any side effect!

At present, the PFC liquid and an oxygen atom is not classified by any country as a controlled medicament matter. Our PFCO-Pharmacy-Machine have provides PFCO-1 and PFCO-2 allows certified medical practitioners to prescribe medicine for lung infections caused by bacteria. For example, according to Hong Kong's section 28 of Pharmacy and Poisons Ordinance, all registered practitioners prescribe and use this type of medicine could be without having to register with the medical and drug regulatory department. Furthermore, those unauthorized hospitals and clinics will not dare to use this practice openly. This is therefore beneficial to the PFCO invention and its patent as it gives them more protection. However, as the usage of this medicine may differ among countries, it is necessary that the retailers of different countries to be aware of this.

These designs according to a patent authorize and copyright to possess simultaneously, so which was strictly forbid to counterfeit!

Represented By:



LZM Patent (liaison) Office
10 Ava Road Ava Tower # 19-07
Singapore 329949
Tel: 65-63533647 Fax: 62585636
E-Mail: lhj@yceec.com
lzmyc@singnet.com.sg
WebSite: www.yceec.com

Yet Chong Electric Company
Blk. C-4, 13/F., Wing Hing Ind. Bldg.,
14 Hing Yip St., Kwun Tong, Kln.
Hong Kong
Tel: 852 2344 0137 Fax 2341 9016
E-Mail: lhj@yceec.com
lzmvc@singnet.com.sg

The effect of medication and ingredients of PFCO-1

- The main ingredients of PFCO-1 for Perfluoro and Ozone to be mixed, the molecular formula to part of the C6F14 and O3.
- Due to the characteristics of Ozone was very unsettled and a characteristic of difficult to store, we are to Point out clinic and hospital who should be to buy our PFCO–Pharmacy-Machines to make up by oneself for clinical to put in use immediately and to enhance the effect of medication, also it could be to be frugal the cost.
- As there is a need to define air as an interface, so SARS infection include flu of any type or pulmonary which they were alike property the ulcer of superficiality and bacterial infection, this is a new medical definition and as well as is our basis of patent invent, it was your belief basis for us too! The revolutionize of lung treatment history that already to start, if you no to identify oneself with it be bound to fall behind!
- The Ozone is a benignancy bactericide it was acknowledged in the world, it could be to destroyed or decomposed a cell wall of germs to oxidize the internal of a cell and to cause death the original body of a cell, however, the PFC is a excellent polymerization liquid of macromolecule and it has zero ozone depletion, the collocation it was a seamless heavenly robe.
- The clinical concentration to consult list below:

Ozone sterilizing in liquid (1ppm= 1mg / L)			
O3 Density	Time	Types of viruses and pathogens	Sterilizing efficiency
10mg/m3	20 mins	Type-B hepatitis surface antigen (HbsAg)	99.99%
0.5 ppm	5 mins	Type-A flu virus	99%
0.13 ppm	30 seconds	Poliomyelitis virus type I (PVI)	100%
0.040 ppm	20 seconds	Coliphage ms2	98%
0.25 ppm	1 mins	SA-H and human-wheel virus type 2	99.60%
* 12.6 ppm	4 mins	Coronaviridae	100%
4 ppm	3 mins	HIV	100%
8mg/m3	10 mins	Mycoplasma, Chlamydia, and other pathogens	99.85%

- This medicine substance to suit with registered doctor to put in use clinical for enter lung to cure SARS, bird flu and flu of anyone germs infect; it was unusual for preserved children of tender age whom they are in virtue of head cold to bring about a high fever to surmount 39° C which was easy to lead to pathological changes to die or the intelligence to descend , this medicine substance could be to bring down a fever immediately and it could be to evaporate and not any vestiges.
- The phthisis was same a type of germs infect of lung, this medicine substance has a specific remedy only.
- This medicine substance could be to washing lung of smoker and pneumoconiosis of aged people, because the single oxygen atom it could be to produced intense oxygenation for the deposit-stain to decomposed.

PFCO-1 a matter needing attention of using medication

The Perfluoro liquid of medicine substance it was to choose the PF-5080 electronic liquid of 3M company of USA with to mix Ozone to manufacture, the liquid was to guaranteed that it is non-irritating to the eyes and skin, and is practically non-toxic orally. The 3M company was further to guaranteed the product also demonstrates very low acute and sub chronic inhalation toxicity and the liquid it has zero ozone depletion potential.

Because the Ozone is not chemical reaction for the macromolecule liquid of PFC, so above the distinguishing characteristic of the PFCO-1 liquid that is not to changed; but the characteristics of Ozone was very unsettled, so there is to take apart the glue bag of air-tight wrapping as soon as, the mark concentration of Ozone it could be to descend, the numerical analysis of ppm which was on behalf of the lethality for germs, the PFCO-1 liquid has a characteristic of fine to evaporated it was especially in the body temperature, as well as it must to regulate the concentration of Ozone in the liquid with it could be to once to kill the germs of lung-cavity and to request clinicians who must to look out.

Although in proportion to the concentration of oxygen it may be upward 15-30ppm or above-mentioned, the PFCO–Pharmacy-Machines could be to adjust the oxygen concentration to reach to surmount the evaporate period which breathe capacity of liquid medicine, even if is this, our proposal is that the lungs be used interchangeably during clinical trial phase while the other lungs can still supply oxygen. This is to ensure safety.

To use the mark concentration of Ozone is 10ppm or still more for an allergic reaction and volatility test are our advice, it's volatility is about three times over for alcohol. Those are to have the PFCO–Pharmacy-Machines's clinic and hospital will be to have abundant clinical experience quickly.

This medicine substance it was to belong to a “ lung-cavity an appetite fluid” and it was to originate in medicine history and inconvenient used for the public, so it does not to go on sale, it only to supply for those have the patent authorized and who must were the register doctor, clinic or hospital use the prescription authority for clinical.

Tracheal Tube For Single Use


(一次性氣管導管的使用)

Propose Using !

To operate in coordination using for the
Clinical Three Channel Valve

Caution and instruction manual:

1. Store in clean, dry condition away from light and avoid freezing and excessive heat;
2. Seat 15mm connector firmly into tracheal tube prior to use;
3. Avoid contact with laser beams or electrosurgery electrodes;
4. To tear open the parcel bagging and take out the Tracheal Tube to join the contact;
5. Using an injector to face the gasbag to fill an little gas to check if puncture of the gasbag;
6. To pump out gas of the gasbag;
7. Start the normal operation to intubate procedure;

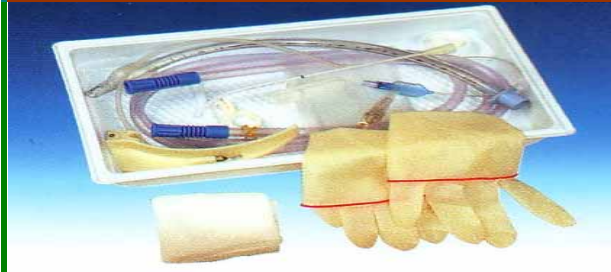

HKD \$30.00

(single tube type)



Children type: 2.5#, 3.5#, 4.5#, 5.5#, 6#;
Adult type: 6.5#, 7.5#, 8#, 8.5#, 9#, 9.5#, 10#;

HKD \$50.00 (repeatedly use)

Clinical Three Channel Valve



Common Tracheal Tube Package
For Single Use

Even tube Tracheal Tube for Single use


high-priced !

Standards Diameter

Children type: 2.5#, 3.5#, 4.5#, 5.5#, 6#;
Adult type: 6.5#, 7.5#, 8#, 8.5#, 9#, 9.5#, 10#;



To propose to put to use the improved of new type below

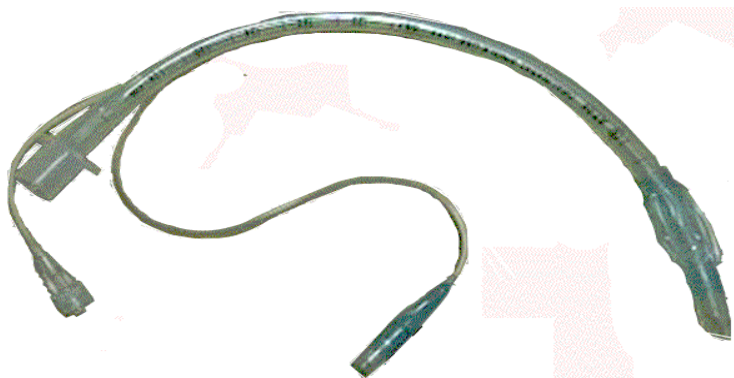

The mouth of fluid infusion

an air lock for to blow